

Excimer Laser Atherectomy for a Long, Diffusely Diseased, Moderately Calcified Right Coronary Artery

OPERATOR / FACILITY

Antonis Pratsos, MD
Bryn Mawr Hospital,
Main Line Health System
Bryn Mawr, Pennsylvania

Case History

- 75-year-old male
- History: Dyslipidemia, insulin dependent diabetes, hypertension with a history of CAD, positive stress test.

Angiography

- Subtotal occlusion
- RCA: Long diffuse disease, moderately calcified
- LAD: Patent with minor luminal irregularities
- Circumflex: 50% stenosis in the mid portion

Intervention

- RCA was engaged with a 6F FR4 guide
- 0.014" Asahi guidewire was inserted into the RCA along with a .014x135 Quick-Cross support catheter to help cross the lesion
- 0.9mm X80 ELCA catheter was used at 50 fluence/40Hz
- PTCA was then performed with a 2.5mm Maverick at 14 ATMs
- Xience 3.0x28 stent was placed in the RCA deployed at 18 ATMS
- PTCA post stent deployment was performed with a 2.50x12mm Quantum Maverick

DEVICES

Guide

- 6F FR4 guide catheter (Boston Scientific®)

Wire

- 0.014" Grandslam Wire® (Asahi®)

Support Catheter

- 0.014"x135cm Quick-Cross® (Spectranetics®)

Lasers

- 0.9mm X80 ELCA® (Spectranetics®)

Balloons

- 2.5x20mm Maverick® (Boston Scientific®)
- 2.5x12mm Quantum Maverick® (Boston Scientific®)

Stents

- 3.0x2.8mm Xience® (Abbott Vascular®)

Anticoagulation

- Angiomax® (The Medicines Company®)

FEATURED SPECTRANETICS PRODUCTS

- ELCA® Coronary Laser Atherectomy Catheter
- Quick-Cross® Support Catheter



RCA Diffuse 1



RCA Diffuse 0.9

Excimer Laser Atherectomy for a Long, Diffusely Diseased, Moderately Calcified Right Coronary Artery


Results / Conclusions

- TIMI 3 Flow
- As demonstrated in this case, laser ablation was performed to treat a moderately calcified long lesion in the RCA
- 0.014x135cm Quick-Cross was used to facilitate the wire crossing the calcified lesion
- The 0.9mm X80 ELCA was used to treat the underlying calcium resulting in easy delivery of balloons & full apposition of the stent


The 0.9mm X80 helped modify the calcium and improved vessel compliance allowing for easy delivery of balloons and stent.

– Antonis Pratsos, MD

At the time of publication, Dr. Pratsos has a consulting agreement with Spectranetics.

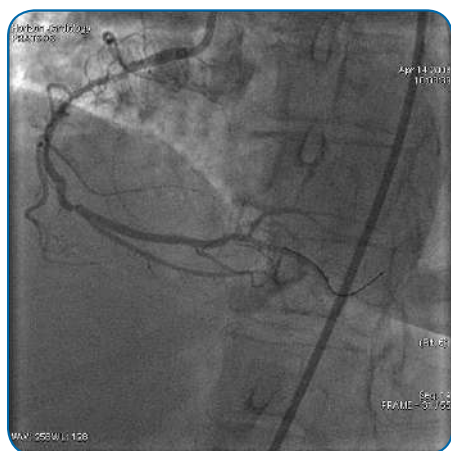

RCA Diffuse Post 0.9

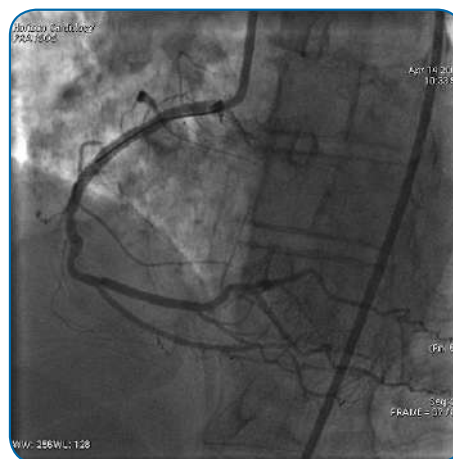

Final RCA Diffuse

Important Safety Information

ELCA® X-80 Coronary Laser Ablation Catheter

INDICATIONS

The X-80 Laser Catheters are intended for use as a stand-alone modality or in conjunction with Percutaneous Transluminal Coronary Balloon Angioplasty (PTCA) in patients who are acceptable candidates for coronary artery bypass graft (CABG) surgery. The following Indications for Use, Contraindications and Warnings have been established through multicenter clinical trials. The Spectranetics CVX-300® Excimer Laser System and the multifiber laser catheter models are safe and effective for the following indications:

- Occluded saphenous vein bypass grafts
- Ostial lesions
- Long lesions – (greater than 20mm in length)
- Moderately calcified stenoses.
- Total occlusions traversable by a guidewire.
- Lesions which previously failed balloon angioplasty - This includes those lesions that were treated unsuccessfully by PTCA. Lesions that have undergone a complicated PTCA procedure are not included in this category.

These lesions must be traversable by a guidewire and composed of atherosclerotic plaque and/or calcified material. The lesions should be well defined by angiography.

CONTRAINDICATIONS

- Patient has acute thrombosis.
- Lesion is in an unprotected left main artery.
- Patient has experienced an acute myocardial infarction.
- Patient has ejection fraction of less than 30%.
- Lesion is beyond acute bends or is in a location within the coronary anatomy where the catheter cannot traverse.
- Guidewire cannot be passed through the lesion.

Quick-Cross® Support Catheter

INDICATIONS

Quick-Cross Support Catheters are guidewire exchange and infusion devices designed for use in the vascular system. The catheters are intended to support a guidewire during access of vasculature, allow for exchange of guidewires and provide a conduit for the delivery of saline solutions or diagnostic contrast agents.

CONTRAINDICATIONS

None known.

See complete IFU for more information before attempting use of Quick-Cross.

ADVERSE EVENTS

Atherectomy or any other surgical procedure has inherent risks. For a completing listing, see the IFU.

- Lesion is located within a bifurcation.
 - Patient is not an acceptable candidate for bypass graft surgery.
- See complete IFU for more information before attempting use of ELCA X-80.

WARNINGS

Federal (USA) law restricts this device to sale by or on the order of a physician with appropriate training. A clinical investigation of the Spectranetics CVX-300® Excimer Laser System did not demonstrate safety and effectiveness in lesions amenable to routine PTCA or those lesions not mentioned in the Indications for Use, above. The effect of adjunctive balloon angioplasty on restenosis, as opposed to laser alone, has not been studied. The use of the CVX-300® Excimer Laser System is restricted to physicians who are trained in the use of the product.

PRECAUTIONS

This device has been sterilized using Ethylene Oxide and is supplied STERILE. The device is designated and intended for SINGLE USE ONLY and must not be re-sterilized and/or reused. Store in a cool, dry place. Protect from direct sunlight and high temperatures (greater than 60°C or 140°F). During the procedure, appropriate anticoagulant and coronary vasodilator therapy must be provided to the patient. Anticoagulant therapy should be administered per the institution's PTCA protocol for a period of time to be determined by the physician after the procedure. Percutaneous Excimer Laser Coronary Atherectomy (ELCA) should be performed only at hospitals where emergency coronary bypass graft surgery can be immediately performed in the event of a potentially injurious or life-threatening complication. The results of clinical investigation indicated that patients with the following conditions are at a higher risk for experiencing acute complications:

- Patients with diabetes.
- Patients with a history of smoking.
- Lesions with tortuous vessels.

WARNINGS

Maximum infusion pressure is 300 psi. The catheter is designed and intended for intravascular use only. This catheter is designed and intended for one-time use only. Do not re-sterilize and/or reuse. Careful inspection before use should verify that the catheter has not been damaged in shipment and that its condition is suitable for the procedure. The catheter should not be advanced through an area of resistance unless the source of resistance is identified by fluoroscopy and appropriate steps are taken to reduce or remove the obstruction. Catheter manipulation should occur only under fluoroscopy. If the catheter is used for infusion, reference the table of flow rates and ensure infusion pressure does not exceed the recommendations. Avoid introducing air or any other gas through the catheter into the vascular system.